





1 Prepare Test

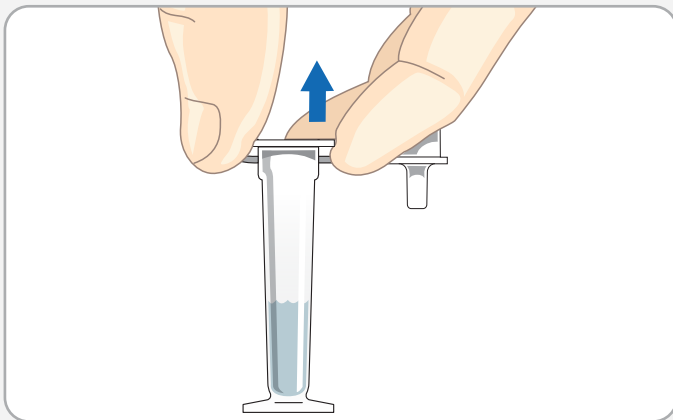


Remove ROM Plus contents from packaging. Holding buffer vial in upright position, remove shipping cap and set it aside.

2 Collect Sample

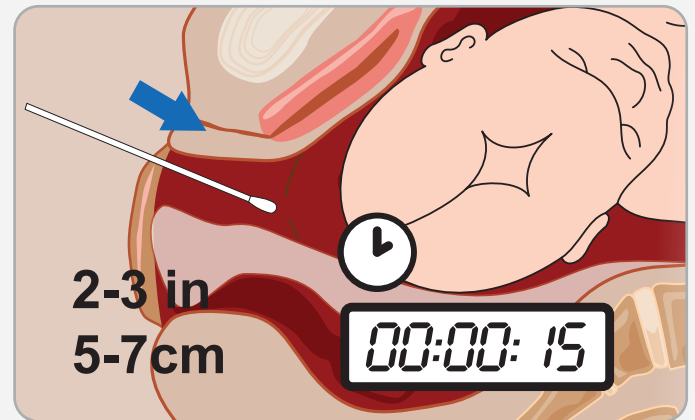


Remove sterile swab from package. Insert the swab tip into the vagina 2-3 inches (5-7 cm). Withdraw the swab after a minimum of 15 seconds.

3 Place Swab in Vial

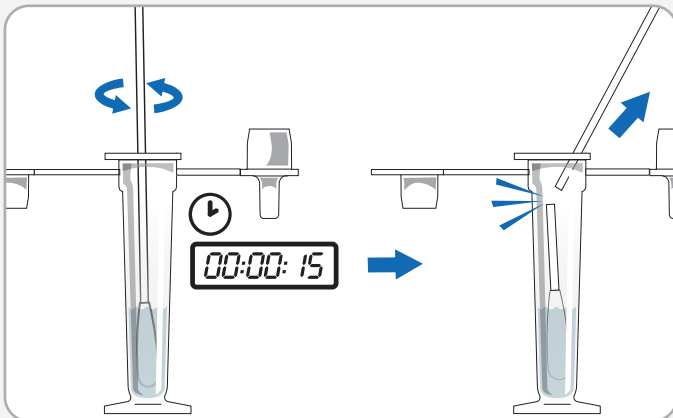


Place swab tip into vial. Mix the swab in the buffer for at least 15 seconds. Break off swab tip and leave tip in vial and dispose of remaining swab stick.

4 Lab or POC

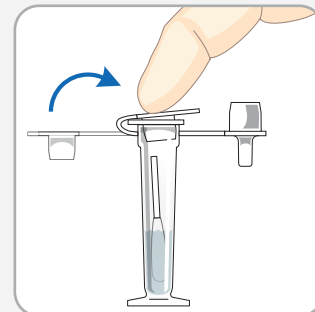

If reading test in lab, place shipping cap back on vial and send to lab.


OR

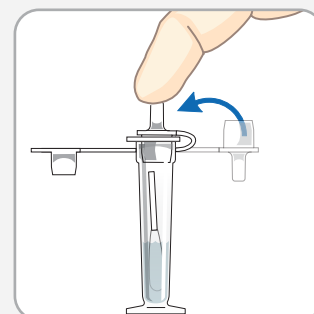

If using test POC, place dropper cap on vial. Skip to **Step 2** on backside.


Quick Reference Guide- Sample Testing

1 Place Dropper Cap

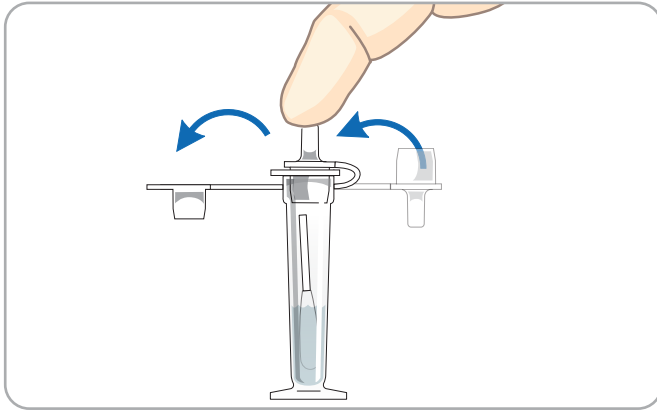


Replace shipping cap with drop dispenser cap.

2 Place Sample into Cassette

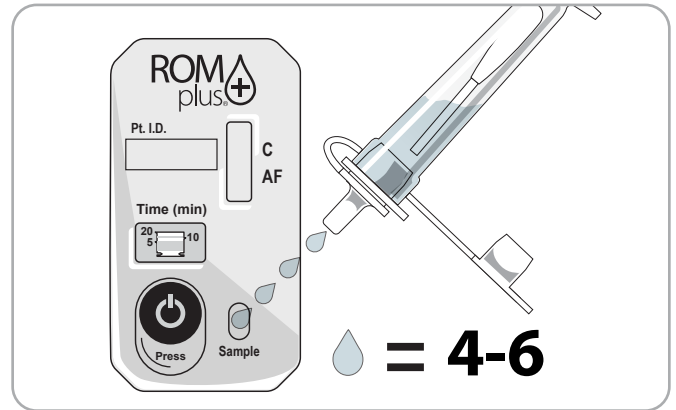


Remove ROM Plus cassette. Add 4-6 drops of sample/ buffer solution to the sample well on the test cassette.

3 Start Timer

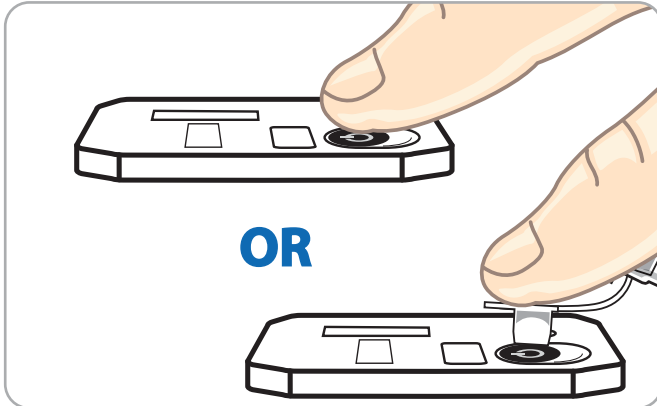


Start timer by firmly pressing and rolling thumb over the timer button, or use the lid on the vial. Timer has been activated when you see dark blue dye in window.

4 Wait 5-20 Minutes

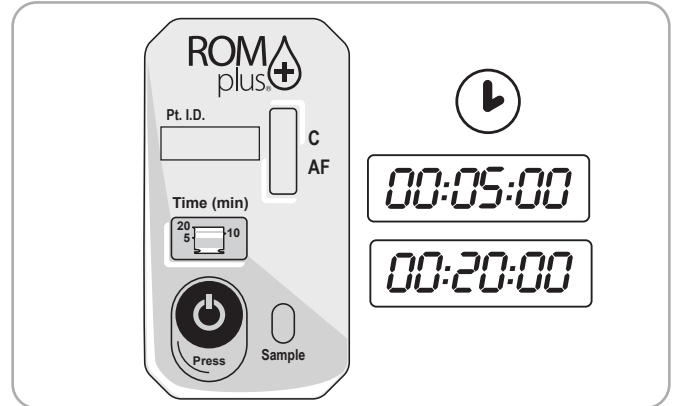

A positive test result may be visible early (within 1-3 minutes) or may take the full 20 minutes. Wait the full 20 minutes to confirm a negative result.

5 Interpret Test Results

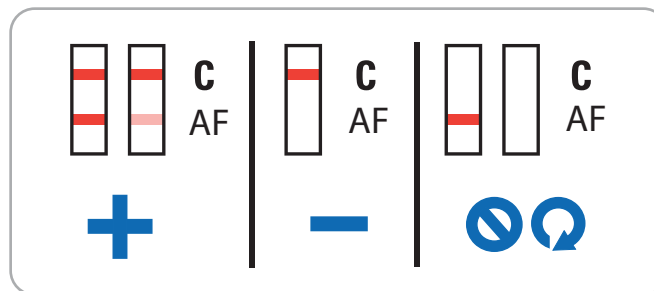

The test is valid even if the lines are faint. Test is positive if two lines (C) and (AF) appear. If no lines are visible, or just the test line (AF) is visible, the test is invalid and should be repeated.

See Package Insert for Full Instructions, Warnings, Precautions & Contraindications

Local Distributor:

clinicalinnovations.com.au

36 Matheson Street, Virginia
Queensland 4014 | Australia
Phone +07 3862 2000 | Fax +07 3862 2077
enquiries@clinicalinnovations.com.au



**CLINICAL
INNOVATIONS
AUSTRALIA**
forMUM. forBABY. forLIFE.™